

Q-NAD BLOOD NAD⁺ and NADH assay kit

Q40 NAD⁺ & NADH Blood Kit (RUO)

Quantitative 40-sample assay kit for whole blood

Version 10.0

FOR SINGLE USE ONLY

These instructions must be read in their entirety before using this product.

RUO

For Research Use Only.
Not for use in diagnostic procedures.

GENERAL INFORMATION

Proprietary name:

Q-NAD Blood NAD⁺ and NADH assay kit: quantitative assay kit for whole blood

Catalog numbers:

RUO_001

RUO_001_US

Storage:

-85° - -70°C upon arrival

IFU issued:

February 2026

Manufacturer:

NADMED Ltd / Oy

www.nadmed.com

info@nadmed.com

Tukholmankatu 8, Biomedicum 2U

00290 Helsinki

FINLAND

SYMBOLS ON THE PACKAGING



Contains flammable liquid and vapor. Refer to PRECAUTIONS AND WARNINGS



Warning/danger. Refer to PRECAUTIONS AND WARNINGS



Consult instructions for usage



Use-by date




Catalogue number



Batch code



Manufacturer




Upper limit of storage temperature



Do not use if package is damaged



Number of reactions



For Research Use Only



Protect from direct light



Keep dry

TABLE OF CONTENTS

GENERAL INFORMATION..... 2

SYMBOLS ON THE PACKAGING 2

INTRODUCTION 4

RESEARCH BACKGROUND 4

PRINCIPLE OF THE ASSAY 4

SAMPLE HANDLING AND STORAGE 5

REAGENT STORAGE, STABILITY, AND PREPARATION..... 6

PRECAUTIONS AND WARNINGS 7

TROUBLESHOOTING 7

MATERIALS REQUIRED BUT NOT PROVIDED IN THE KIT 8

PRACTICAL CONSIDERATIONS..... 9

WORKFLOW OF Q-NAD BLOOD NAD+ AND NADH ASSAY 10

EXTRACTION AND STABILIZATION OF NAD+ AND NADH..... 11

PREPARATION OF STANDARDS 13

PREPARATION OF POSITIVE CONTROL..... 14

ASSAY PROCEDURE..... 15

CALCULATION OF RESULTS 17

PERFORMANCE AND LIMITATIONS 20

NOTES..... 22

PLATE LAYOUT..... 23

INTRODUCTION

NAD metabolites are derivatives of vitamin B3 and exist in cells in four forms – NAD⁺, NADH, NADP⁺, and NADPH. NAD metabolites are essential for the functional adaptation of cell metabolism to environmental conditions. Their levels are dynamic and change in response to different endogenous and exogenous stimuli. This kit is designed for the separate measurement of systemic levels of NAD⁺ and NADH in whole blood (human or animal).

RESEARCH BACKGROUND

NAD⁺ and NADH metabolites play a pivotal role in adjusting human metabolism and energy homeostasis in response to various internal and external stimuli. Research has demonstrated that systemic NAD⁺ levels diminish in correlation with the onset of diseases, signaling a disruption in the body's energy equilibrium (Covarrubias et al. 2021 doi: [10.1038/s41580-020-00313-x](https://doi.org/10.1038/s41580-020-00313-x)). The extent of this NAD⁺ reduction is not uniform and varies across different individuals and pathologies. A significant decline in NAD⁺ impairs the body's ability to sustain essential metabolic functions, a condition that persists even with ongoing therapy. Ongoing research on the contribution of NAD⁺ and NADH to the mechanisms and progression of different diseases is very active. A list of pathologies with suspected changes in NAD⁺ and NADH concentrations is constantly expanding with already published evidence for mitochondrial disease, aging, sepsis, viral infections, cardiovascular and kidney disease, diabetes types I and II, neurological disorders, and cancer (e.g., Pirinen et al. 2020 doi: [10.1016/j.cmet.2020.04.008](https://doi.org/10.1016/j.cmet.2020.04.008), Verdin 2015 doi: [10.1126/science.aac4854](https://doi.org/10.1126/science.aac4854), Fan et al 2020 doi: [10.1111/jdi.13303](https://doi.org/10.1111/jdi.13303), Navas & Carnero 2021 doi: [10.1038/s41392-020-00354-w](https://doi.org/10.1038/s41392-020-00354-w)).

PRINCIPLE OF THE ASSAY

The kit measures intracellular NAD⁺ and NADH content. The principle of the assay is a cyclic enzymatic reaction with a colorimetric end-point detection. First, NAD⁺ and NADH metabolites are extracted together from a whole blood sample in a single step. In the analytical process, the sample extract undergoes separate measurements for NAD⁺ and NADH. In the first segment, the procedure focuses on stabilizing NAD⁺ while actively eliminating NADH. Conversely, in the second segment, the emphasis shifts to stabilizing NADH, concurrently ensuring the removal of NAD⁺. The NAD⁺ and NADH stabilized extracts are analyzed on two separate plates by an enzymatic reaction coupled with a color change. The intensity of the color change in the assay is linearly proportional to the concentration of NAD⁺ or NADH in the reaction mixture.

SAMPLE HANDLING AND STORAGE

Requirements and Limitations:

- This kit is designed for NAD⁺ and NADH measurement in whole blood. This assay is NOT suitable for measuring in plasma or serum, cultured cells, or tissues.
- For measuring NAD⁺ and NADH, 100 µL of whole blood is needed. However, a volume of 150–200 µL is optimal to perform the assay reliably.
- Samples can be analyzed either fresh or frozen.
 - a) Fresh blood can be analyzed within 72 hours after collection. After withdrawal, store at 4°– 8°C until analysis.
 - b) Once frozen, samples must be kept frozen before the assay. Subsequent freeze-thaw cycles are not allowed. Storage time for frozen samples is one month at -20°C, or one year at -80 – -70°C.
- In clinical trials and longitudinal studies, it is important to have consistent pre-analytic practices. Aim for consistency in sampling, handling, storage, and analysis type (fresh or frozen). Refer to the Blood collection instructions and Important precautions below.

Blood collection:

Collection: Whole blood samples taken from a vein (using methods like venipuncture) and whole blood samples taken from other parts of the body (using a lancet-type device) are suitable. Detailed instructions on aliquoting and freezing blood samples can be found at <https://www.nadmed.com/documents/>.

Sample volume: The analysis itself requires small volumes of whole blood. Thus, if analyzing frozen samples, we recommend aliquoting a larger volume of blood (e.g., 2–3 mL) into 150–200 µL aliquots before freezing. Collecting the blood directly into a collection tube with anticoagulants is vital to keep the target concentration of anticoagulant in the sample.

Anticoagulants: In general, whole blood samples should be collected into collection tubes with K2 EDTA or Lithium heparin (LH) as anticoagulants and properly mixed by up-and-down rotation. Final concentrations of anticoagulants should be 1.2–2 mg of K2 EDTA per 1 mL of collected blood, or 17–18 IU of LH per 1 mL of collected blood. For venous blood collection, we recommend blood collection vacutainers with a spray coating of K2 EDTA or LH designed to result in anticoagulant concentrations described above (e.g., BD Vacutainer® or Vacuette®).

Important precautions to ensure the integrity and reliability of the results:

Mixing the Sample: When whole blood remains stationary, it separates into different phases. During processing, a fresh sample should be thoroughly and frequently mixed.

Timing of Analysis and Aliquoting: If you cannot analyze the blood sample immediately after collection, make sure to divide (=aliquot) the sample within 72 hours into the preferred volume of 150–200 µL.

Storing aliquots: Store the aliquots in non-sterile, single-wall transparent polypropylene microtubes. The tubes should have a capacity of 0.5 to 2 mL. After aliquoting, freeze the samples quickly. Use pre-cooled sample containers in temperatures from -80°C to -20°C for freezing.

Practices to avoid: Do not freeze large (2–3 mL) volumes of blood directly in the collection tubes. Do not use skirted double-wall microtubes. These practices can significantly increase the time needed to freeze and thaw. Long freezing/thawing times can cause variability in assay results, affecting the accuracy and reliability of the analysis.

REAGENT STORAGE, STABILITY, AND PREPARATION

Before opening, all kit components should be stored at -85°C - -70°C. Avoid temperature fluctuations in the freezer.

REAGENT	DESCRIPTION (*)	PREPARATION (**)	STABILITY (**)
EXTRACTION BUFFER A	28 mL Sufficient for 40 samples	Equilibrate to room temperature. Ready for use.	Stable for two weeks at room temperature after thawing.
NAD+ STABILIZER	8 mL Sufficient for 40 samples		
NADH STABILIZER	8 mL Sufficient for 40 samples		
POSITIVE CONTROL (BUFFER)	200 µL Sufficient for two plates		
DEIONIZED WATER	10 mL Sufficient for two plates		
STOP SOLUTION	3 mL Sufficient for two plates	Equilibrate to room temperature. Ready for use. (If precipitates have formed, warm the solution to +37°C, then cool to room temperature before the assay.)	Stable for 12 hours at room temperature after thawing. Keep in the amber bottle.
ASSAY BUFFER C	2x 19 mL One aliquot per 96-well plate	Equilibrate to room temperature. ASSAY BUFFER C + ASSAY COLOR REAGENT = Assay Master Mix.	
ASSAY COLOR REAGENT	2x 3 mL One aliquot per 96-well plate	See preparation guide on page 15.	Stable for 3 hours at room temperature after thawing. Keep in the amber bottle.
NAD+ STANDARD STOCK	40 µL (1mM) Sufficient for Standards and Positive control	See preparation guide on page 13.	Should be used immediately after thawing. Should be protected from light.
NADH STANDARD STOCK	40 µL (1mM) Sufficient for Standards and Positive control		
NAD ENZYME	2x 40 µL One aliquot per 96-well plate	Add to the Assay Master Mix only after processing of plate blanks.	Should be used immediately after thawing.

*Accepted variation of the filling volume +/-5%.

** Room temperature: 15-25°C

PRECAUTIONS AND WARNINGS

For research use only. For trained personnel use only. Do not smoke, drink, eat, or apply cosmetics in the working area. Wear protective gloves, clothing, and eye protection. Wash hands thoroughly after handling.

EXTRACTION BUFFER A may cause eye irritation. Handle with care; use goggles.

NAD⁺ STABILIZER may cause skin and eye irritation. Handle with care; use gloves and goggles.

NADH STABILIZER may cause skin, eye, and respiratory irritation. Avoid inhaling fumes.

STOP SOLUTION may cause skin, eye, and respiratory irritation. Avoid inhaling fumes.

ASSAY COLOR REAGENT may cause skin irritation. Handle with care; use gloves.

The Q-NADMED Safety Data Sheet ([SDS](#)) presents the identified hazards of the chemicals in this kit and the appropriate warning information associated with those hazards.

The Q-NADMED Safety Data Sheet ([SDS](#)) describes the disposal of used kit components.

TROUBLESHOOTING

If you encounter any issues during extraction or assay performance, refer to the NADMED troubleshooting guide at <https://www.nadmed.com/documents/>.

MATERIALS REQUIRED BUT NOT PROVIDED IN THE KIT

CATEGORY	ITEM	SPECIFICATIONS/REQUIREMENTS
Consumables	Microtubes, 1.5 mL	Use non-sterile microcentrifuge tubes made from transparent/natural color polypropylene (PP) intended for <i>in vitro</i> diagnostics (e.g., Sarstedt ref. 72.690.001). <u>NOT</u> compatible with NADMED assay: a) molecular biology grade sterile microtubes that are free of endotoxin, pyrogen, human DNA, and low retention (chemically sterilized) b) microtubes intended for protein work marked "LoBind"
	96-well plates (2 pieces)	Use non-sterile, transparent, polystyrene flatbottom plates with medium protein binding intended for colorimetric assays (e.g. Revvity, ref. 6055640).
	Liquid reservoirs for multichannel pipetting (2 pieces)	Use non-sterile polystyrene plastic. Use separate reservoirs for Assay Master Mix and STOP SOLUTION.
	Pipette tips	Use non-sterile, bevelled pipette tips with low retention.
	Ice (Ice-water bath)	Fill a container with packed laboratory ice and pour cold tap water to reach to a slush-like state. The added water is sufficient when the liquid part of the sample is immersed in water but the ice firmly holds the inserted tubes upright (avoid samples floating in the water).
	Aluminium foil	Use foil covers to protect samples, standards, and the plates from light during assay performance as indicated in the instructions.
Equipment and Machinery	Calibrated Pipettes	Single channel for volumes of e.g. 5-50 µL, 20-200 µL, and 100-1000 µL. Multichannel pipettes for volumes of e.g. 5-50 µL and 30-300 µL.
	Microcentrifuge	Use centrifuge with cooling to +4°C and speed up to 20,000 x g
	Spectrophotometric Microplate Reader	a) Capable to measure absorbance at 570-573 nm wavelength b) Adjustable scanning brightness/intensity. Select "low", or alternatively, adjust the brightness based on the number of flashes per measurement to 5-10 flashes.
	Dry bath Heat Block fitted for 1.5 mL Microtubes	Adjustable temperature up to 80°C is required. To ensure consistent and reliable results, test the heat transfer and calibrate the time needed to reach target temperature: 1. Set your heat block at 80°C and wait until it reaches 75-80°C. 2. Add 500 µL of water into a microtube and place the tube on your heat block. Make sure the microtube fits tightly to the block. 3. Insert a conventional lab thermometer into the microtube with water. 4. Measure the time needed to reach 75°C. The heat transfer is considered sufficient if the temperature is reached within 5 minutes. If the correct temperature is NOT reached with 80°C setting in 5 minutes: a) ensure the tubes fit the block tightly b) increase the target temperature of your device. Recalibrate.
Special	Possibility to work in dim light conditions for the ASSAY part of the measurement. Refer to PRACTICAL CONSIDERATIONS and WORKFLOW OF Q-NAD BLOOD NAD+ AND NADH.	


PRACTICAL CONSIDERATIONS

 Please refer to (<https://www.nadmed.com/products/NAD-NADH-kit>) for visual instructions.


CATEGORY	INSTRUCTIONS
Limitations	Read the SAMPLE HANDLING AND STORAGE carefully. This assay is designed for whole blood and is NOT suitable for measuring NAD⁺ and NADH in plasma or serum, cultured cells, or tissues. Do not use kit components beyond the expiry date. Do not mix materials from different kit lots. Subsequent freeze-thaw cycles of reagents are not allowed.
Usability	Thoroughly mix all reagents by gentle swirling. Small microtubes should be quickly centrifuged at low speed before opening. We recommend taking the DEIONIZED WATER, EXTRACTION BUFFER A, NAD⁺ STABILIZER, NADH STABILIZER, and STOP SOLUTION to room temperature one day before the assay. Take ASSAY BUFFER C and ASSAY COLOR REAGENT to room temperature on the day of the assay. These bottles take about 2-3 hours to melt.
Accuracy	The analyses of NAD⁺ and NADH are done on two separate plates. We recommend performing both assays on the same day. To avoid cross-contamination, change to new pipette tips between the additions of each standard, samples, and reagents. Avoid touching the content of the wells with pipette tips when working with multi-channel pipettes. High-precision pipettes and beveled tips with less retention will improve the precision. ASSAY BUFFER C and STOP SOLUTION contain detergents. To avoid bubbles, pipette the Master mix and STOP SOLUTION by pressing the pipette to the first stop position only. Remove any bubbles in the wells with a small needle before inserting the plate into the plate reader.
Protection from light	Protect the stabilized sample extracts, standards, and positive controls from light when they are not being actively processed. However, for convenience, extraction, preparation, and pipetting of them onto the 96-well plates can be performed under normal light conditions. ASSAY COLOR REAGENT is a yellow, light-sensitive compound that turns brown upon enzymatic reaction of the assay. Exposure to excess natural light or direct artificial light causes unspecific color change to green. To minimize the light interference with the assay, the protocol indicates the steps specifically requiring dim conditions. To protect the reactions from both natural and direct artificial light, we recommend the following: • Switch off artificial light source directly above your bench. Close blinds or move further away from a window. • Use aluminum foil covers for the plate and pipetting reservoirs whenever working with ASSAY COLOR REAGENT and Assay Master Mix. • Cover the 96-well plates with aluminum foil covers during Assay incubation steps until the plate is inserted into plate reader. (Do not wrap).

WORKFLOW OF Q-NAD BLOOD NAD⁺ AND NADH ASSAY

1. Extraction of Metabolites and NAD⁺/NADH stabilization

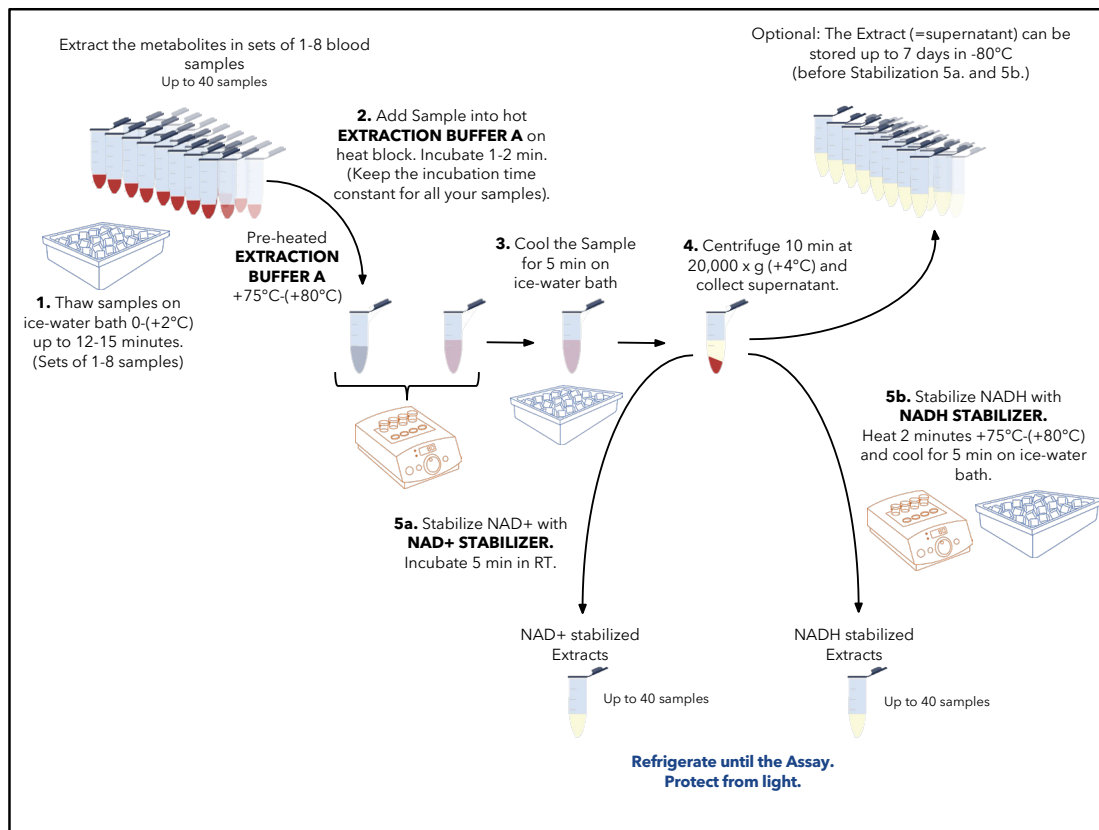

2. Preparation of NAD⁺/NADH Standards and NAD⁺/NADH Positive Controls 3. NAD⁺ and NADH Assays

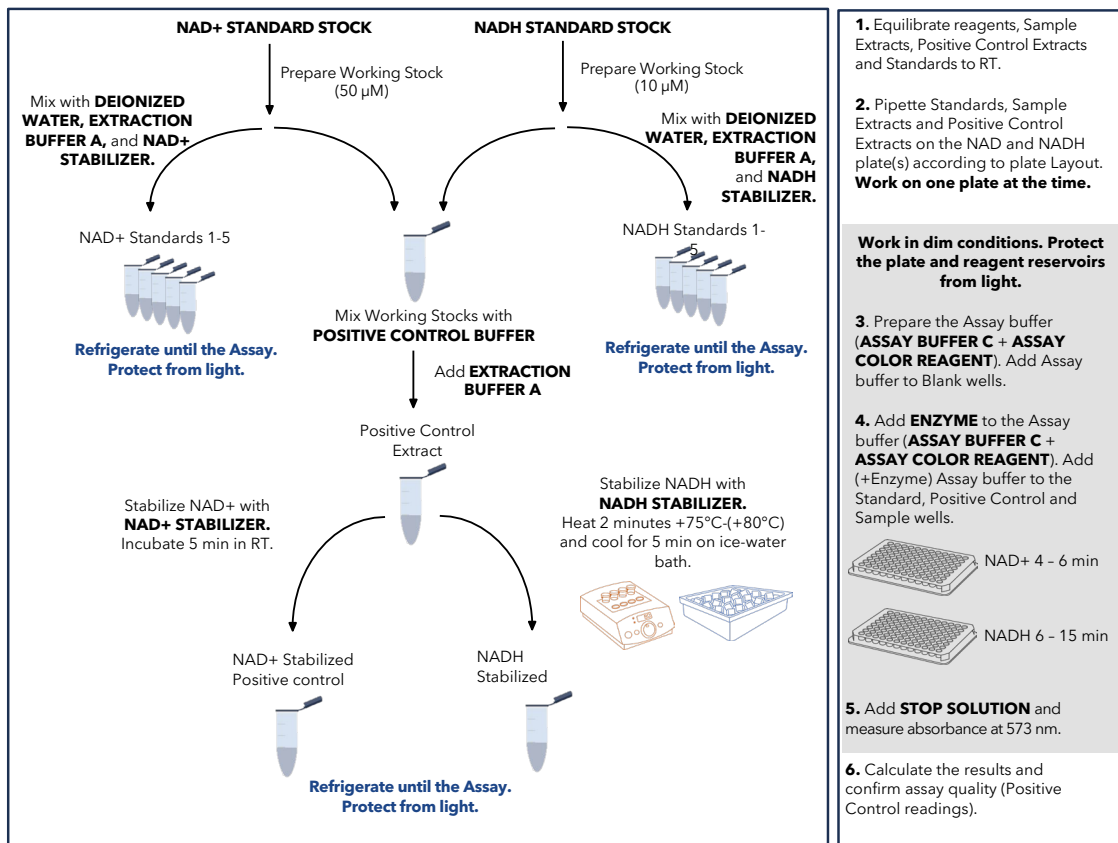

EXTRACTION AND STABILIZATION OF NAD⁺ AND NADH

This section provides guidance on the extraction of NAD⁺ and NADH from whole blood. Following their extraction, NAD⁺ and NADH are individually stabilized in preparation for separate colorimetric assays. Extracts (after centrifugation) can be stored at -80°C - -70°C for one week before stabilization on the day of assays.

TIP: Please refer to video guidance (<https://www.nadmed.com/products/NAD-NADH-kit>)

NOTE: Final dilution of the original whole blood sample will be 10 times. In the case of supplementation with NAD-precursors, the levels of NAD⁺ may increase in the subject's blood. Thus, the NAD⁺ stabilized extract should be further diluted 1:2 using DEIONIZED WATER (provided) before the colorimetric assay. In this case, the dilution of the original blood sample will be 20 times for NAD⁺. The NADH-stabilized extracts do not require dilution.

Materials:

Dry bath heat block set at 75°-80°C	Refer to MATERIALS REQUIRED-Table
Ice-water bath	Refer to MATERIALS REQUIRED-Table
Microcentrifuge	Refer to MATERIALS REQUIRED-Table
Microtubes	Marked for all steps
EXTRACTION BUFFER A	Room temperature
NAD ⁺ STABILIZER	Room temperature
NADH STABILIZER	Room temperature
DEIONIZED WATER	Room temperature

Extraction:

1. Pipette 500 µL of **EXTRACTION BUFFER A** into 1.5 mL microtubes for all your samples. Close the caps.
2. a) If you work with fresh blood samples, proceed to extraction with EXTRACTION BUFFER A.
b) If you work with frozen whole blood samples, thaw them in the ice-water bath as follows:
 - Work with sets of 1-8 samples at a time.
 - During the first minutes of thawing, remove any ice that has formed on the tube walls.
 - Thawing should be completed within 12-15 minutes. Monitor the thawing and facilitate it if necessary: hold the sample for 2-3 seconds and place it back in the ice-water bath, repeat every 2 minutes.
3. Pre-heat EXTRACTION BUFFER A (in sets of 1-8 samples) in the dry bath heat block set to 80°C for the time needed to reach the target temperature within 75-80°C (see section MATERIALS REQUIRED).
4. Mix the thawed whole blood sample with a few up-and-down pipetting cycles; avoid foaming.
5. Without removing the EXTRACTION BUFFER A microtube from the heat block, inject the sample as follows:
 - Pipette 100 µL of blood into the EXTRACTION BUFFER A without touching the bottom of the tube.

- Quickly mix with 5-7 intensive up-and-down pipetting cycles and simultaneous rotation of the tip for efficient mixing of the cold sample and hot EXTRACTION BUFFER A.
6. Incubate each reaction at 75°-80°C for 1-2 min. Keep the incubation time constant for all your samples.
 7. Cool down the extract in the ice-water bath for at least 5 min. Check the sample for successful extraction. After cooling on ice, homogenate should polymerize without any free liquid.
- ↻ Repeat the extraction for the next batch(es) of 1-8 samples.
8. Centrifuge the extracts at 20,000 x g at 4°C for 10 min. Transfer the supernatant into a clean microtube and discard the pellet.
 9. Protect the sample extracts (supernatants) from light and keep them refrigerated (4°-8°C) for **up to 1h before proceeding to the Stabilization steps.**
- Optional: The supernatants can be stored at -80°C - -70°C for one week. In this case, thaw the frozen extracts at room temperature for 10 min before proceeding to the stabilization steps described below.

Stabilization:

10. Equilibrate the extract to room temperature and prepare two 150 µL aliquots into clean microtubes.
11. To the first 150 µL aliquot, add 100 µL of **NAD+ STABILIZER**. Vortex, and incubate at room temperature for 5 min.
12. To the second 150 µL aliquot, add 100 µL of **NADH STABILIZER**. Vortex, and incubate for 2 min in a dry-bat set at 80°C. Cool down on ice for 5 min.
13. Protect Stabilized sample extracts from light and keep them refrigerated (4°-8°C) before pipetting on the Assay plates.

PREPARATION OF STANDARDS

Prepare standards on the day of the assay. Prepare one standard set at a time, starting with NAD⁺. The working standard stocks prepared here are used to prepare the Positive control mix.

NOTE: Use the same pipette for DEIONIZED WATER and Standard working stocks to improve accuracy.

Materials:

1 mM NAD ⁺ STANDARD STOCK	Thaw upon usage. Spin down at low speed before opening
1 mM NADH STANDARD STOCK	Thaw upon usage. Spin down at low speed before opening
EXTRACTION BUFFER A	Room temperature
NAD ⁺ STABILIZER	Room temperature
NADH STABILIZER	Room temperature
DEIONIZED WATER	Room temperature

Protocol:

1. Thaw microtubes with 1 mM NAD⁺ STANDARD and 1 mM NADH STANDARD for 5 min at room temperature. Protect from light with a foil lid during thawing.
2. Prepare **50 µM NAD⁺ working stock** by adding 25 µL of 1 mM NAD⁺ STANDARD STOCK into 475 µL of DEIONIZED WATER, vortex. Proceed to the preparation of NAD⁺ standards according to the table below, pipette the reagents in the indicated order.

NAD ⁺ STANDARD PREPARATION:					
STANDARD ID	NAD ⁺ CONCENTRATION (µM)	DEIONIZED WATER (µL)	50 µM NAD ⁺ working stock (µL)	EXTRACTION BUFFER A (µL)	NAD ⁺ STABILIZER (µL)
NAD ⁺ ST1	0	100	0	500	400
NAD ⁺ ST2	1	80	20	500	400
NAD ⁺ ST3	2	60	40	500	400
NAD ⁺ ST4	3	40	60	500	400
NAD ⁺ ST5	5	0	100	500	400

3. Prepare **10 µM NADH working stock** by adding 10 µL of 1 mM NADH STANDARD STOCK into 990 µL of DEIONIZED WATER, vortex. Proceed to the preparation of NADH standards according to the table below, pipette the reagents in the indicated order.

NADH STANDARD PREPARATION:					
STANDARD ID	NADH CONCENTRATION (µM)	DEIONIZED WATER (µL)	10 µM NADH working stock (µL)	EXTRACTION BUFFER A (µL)	NADH STABILIZER (µL)
NADH ST1	0.0	100	0	500	400
NADH ST2	0.2	80	20	500	400
NADH ST3	0.4	60	40	500	400
NADH ST4	0.6	40	60	500	400
NADH ST5	1.0	0	100	500	400

4. Vortex all Standards. Protect the Standards from light and keep them refrigerated (4°-8°C) before pipetting on the Assay plates.

PREPARATION OF POSITIVE CONTROL

The Positive control is mimicking the level of NAD metabolites in a blood sample of a healthy human subject. Positive control undergoes extraction and stabilization like the whole blood samples. The expected concentration of NAD⁺ in the Positive control is $25 \pm 2 \mu\text{M}$, and NADH is $2 \pm 0.3 \mu\text{M}$ after calculation of results.

NOTE: The Positive control is prepared right after the preparation of the Standards due to the limited stability of $10 \mu\text{M}$ NADH working stock.

Materials:

Dry bath heat block set at 75°–80°C	Refer to MATERIALS REQUIRED-Table
Ice-water bath	Refer to MATERIALS REQUIRED-Table
50 μM NAD ⁺ working stock	From Preparation of standards, room temperature
10 μM NADH working stock	From Preparation of standards, room temperature
POSITIVE CONTROL (BUFFER)	Room temperature
EXTRACTION BUFFER A	Room temperature
NAD ⁺ STABILIZER	Room temperature
NADH STABILIZER	Room temperature

Protocol:

1. Prepare the Positive control mix in a microtube. Vortex.
45 μL of **POSITIVE CONTROL (BUFFER)**
75 μL of **50 μM NAD⁺ working stock**
30 μL of **10 μM NADH working stock**
2. Pipette 500 μL of **EXTRACTION BUFFER A** into a clean microtube.
3. Add 100 μL of Positive control mix into the EXTRACTION BUFFER A. Vortex.

NOTE: Positive control is extracted with EXTRACTION BUFFER A at room temperature; no heating is needed.

4. Prepare two 150 μL aliquots of the Positive control extract into clean microtubes.
5. To the first 150 μL aliquot, add 100 μL of **NAD⁺ STABILIZER**. Vortex, and incubate at room temperature for 5 min.
6. To the second 150 μL aliquot, add 100 μL of **NADH STABILIZER**. Vortex, and incubate for 2 min in a Dry bath heat block at 80°C. Cool down on ice for 5 min.
7. Protect the stabilized NAD⁺ and NADH Positive control extracts from light and keep them refrigerated (4°–8°C) before pipetting on the Assay plates.

ASSAY PROCEDURE

The Assay procedure is the same for both NAD⁺ and NADH measurements.

Blanks are used to correct for unspecific background signals from unspecific interactions between the extract components and the ASSAY COLOR REAGENT in the Master mix. Sample blanks are incubated with Master mix without added NAD ENZYME. Positive control does not require a separate blank. Sample blanks are to be prepared at a minimum from four representative stabilized sample extracts. If the analyzed subjects have records of NAD supplementation, we recommend using samples with and without supplementation as blanks (two wells per condition, at minimum).

NOTE: Steps 1.-2. are performed under normal light conditions. **Steps from 3. onwards are performed in dim conditions (refer to PRACTICAL CONSIDERATIONS: Protection from light).**

NOTE: The color intensity in NADH assay is generally lower than in NAD⁺ due to lower concentration of NADH in the Standards and whole blood. Follow the suggested incubation times for NAD⁺ and NADH. However, the reaction can be stopped when there is a distinct color gradient in the standards and differences in color intensity between samples with added enzyme and sample blanks. The longer the reaction time, the more intensive the signal observed.

NOTE: Use a separate reservoir for the Master Mix and STOP SOLUTION.

Materials:

Spectrophotometric Reader	Refer to MATERIALS REQUIRED-Table
ASSAY BUFFER C	Room temperature
ASSAY COLOR REAGENT	Room temperature
NAD ENZYME	Thaw upon usage. Spin down at low speed before opening.
STOP SOLUTION	Room temperature

Protocol (Perform the NAD⁺ and NADH assays on separate plates. Work on one Assay at a time):

1. Equilibrate the Standards, Stabilized sample extracts, and Stabilized Positive controls for 10 min at room temperature before pipetting onto the plate.
2. According to the recommended plate layout (see next page), pipette on the 96-well plate:
20 µL Standards (ST1-5) in duplicates
20 µL of stabilized Positive control and Stabilized sample extracts in duplicates (Unknowns, UNK)
20 µL of selected blanks (BL UNK1-4) as instructed above.

NOTE: From this step onward, work in dim conditions.

3. Prepare the Master mix by adding **ASSAY COLOR REAGENT** into **ASSAY BUFFER C**; mix gently by rotation.

NOTE: Protect the Master mix in the reservoir and plate during pipetting with an aluminum foil lid.

- Add 190 μ L of the Master mix WITHOUT NAD ENZYME into each of the four sample blank wells (BL UNK1–4).
- Add 40 μ L of NAD **ENZYME** into the bottle with the remaining Master mix. Mix gently, avoid foaming. Pour the Master mix with the added enzyme into the reservoir.
- Add 190 μ L of the Master mix WITH NAD ENZYME to all remaining wells using a multichannel pipette. Avoid foaming and light. Immediately cover the ready plate with the aluminum foil lid.
- NAD⁺ assay:** Incubate the covered plate for 4–6 min at room temperature.
NADH assay: Incubate the covered plate for 6–15 min at room temperature.
- Stop the reactions by adding 10 μ L of **STOP SOLUTION** to each well in the same order as the Master mix using a multichannel pipette. Avoid foaming. Gently shake the plate by hand on a table surface and remove any bubbles with a needle.
- Measure light absorbance at 573 nm immediately after adding STOP SOLUTION. If possible, shake the plate inside the microplate reader for 5 sec before the measurement.

NOTE: After adding STOP SOLUTION, the color intensity can uniformly increase in all the wells. This is expected due to the non-enzymatic background process in the Master mix.

RECOMMENDED PLATE LAYOUT FOR NAD⁺ OR NADH MEASUREMENTS

1	2	3	4	5	6	7	8	9	10	11	12
St1	St1	UNK1	UNK1	UNK9	UNK9	UNK17	UNK17	UNK25	UNK25	UNK33	UNK33
St2	St2	UNK2	UNK2	UNK10	UNK10	UNK18	UNK18	UNK26	UNK26	UNK34	UNK34
St3	St3	UNK3	UNK3	UNK11	UNK11	UNK19	UNK19	UNK27	UNK27	UNK35	UNK35
St4	St4	UNK4	UNK4	UNK12	UNK12	UNK20	UNK20	UNK28	UNK28	UNK36	UNK36
St5	St5	UNK5	UNK5	UNK13	UNK13	UNK21	UNK21	UNK29	UNK29	UNK37	UNK37
PosCtr	PosCtr	UNK6	UNK6	UNK14	UNK14	UNK22	UNK22	UNK30	UNK30	UNK38	UNK38
BL UNK1	BL UNK2	UNK7	UNK7	UNK15	UNK15	UNK23	UNK23	UNK31	UNK31	UNK39	UNK39
BL UNK3	BL UNK4	UNK8	UNK8	UNK16	UNK16	UNK24	UNK24	UNK32	UNK32	UNK40	UNK40

Plate layout for NAD⁺ or NADH assays: St = standard, BL = Sample blank, PosCtr = stabilized Positive control, UNK = stabilized samples with unknown metabolite concentration. Note that the BL (Sample blanks) of the selected samples are analyzed in the Master mix without added NAD ENZYME.

CALCULATION OF RESULTS

POSITIVE CONTROL (ASSAY QUALITY CONTROL)

Positive control is not a reference, but it aims to monitor the efficiency of the NAD⁺ and NADH stabilization and the colorimetric assay. Before calculating your sample results, confirm that your Positive controls perform as expected.

NAD⁺:

In an NAD⁺ assay, the amount of light absorbed by the stabilized NAD⁺ Positive control should be within the range observed for standards ST3 and ST4. This absorbance range corresponds to an NAD⁺ concentration of 23-27 μM (after correction of 10x dilution).

NADH:

In an NADH assay, the amount of light absorbed by the stabilized NADH Positive control should equal ST2 (+/-0.05 optical units). This absorbance corresponds to an NADH concentration of 1.7-2.3 μM (after correction of 10x dilution).

SAMPLE RESULTS

Calculate results from each plate separately as instructed below. The TYPICAL DATA section below presents examples of standard curves and the calculation of results for control subjects.


1. Calculate the average of the absorbance readings for each standard (ST1-ST5).
2. Create a standard curve by plotting the mean absorbance for each Standard on the y-axis against the known Standard concentration (in μM) on the x-axis. Calculate a simple linear regression fitting of the standard curve.
3. Using the formula of linear regression for the standard curve, calculate the concentration in each of the Sample and Blank wells (UNK and BL UNK).
4. Calculate the average of duplicates of each stabilized sample extract.
5. Calculate the average of the sample blanks (BL UNK1-4). The obtained value represents an unspecific signal of the stabilized extract used for sample normalization.
6. Correct for unspecific signals by subtracting the average of blanks from the average of sample concentrations.
7. Multiply by 10 to obtain the concentration (μM) of NAD⁺ and NADH in blood.

NOTE: If the NAD⁺ stabilized extracts have been additionally diluted due to known supplementation usage, the concentration must be multiplied by the additional dilution factor.

TYPICAL DATA


The standard curve and the concentrations in the stabilized sample extracts are provided for demonstration only and should never be used instead of the real-time calibration curve.

A) STANDARD CURVE FOR NAD⁺

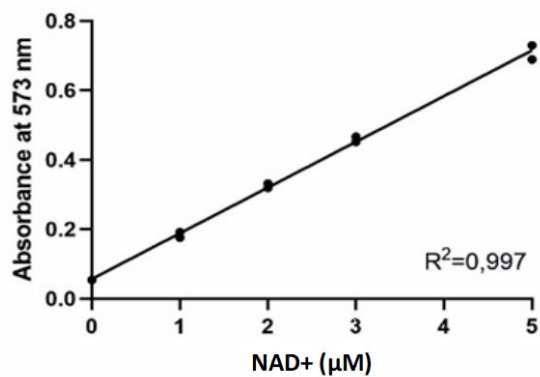

Standard	NAD+ (μM)	Absorbance (573 nm)
Assay time: 4 min		
ST1	0	0.054
ST2	1	0.176
ST3	2	0.319
ST4	3	0.452
ST5	5	0.689

B) STANDARD CURVE FOR NADH

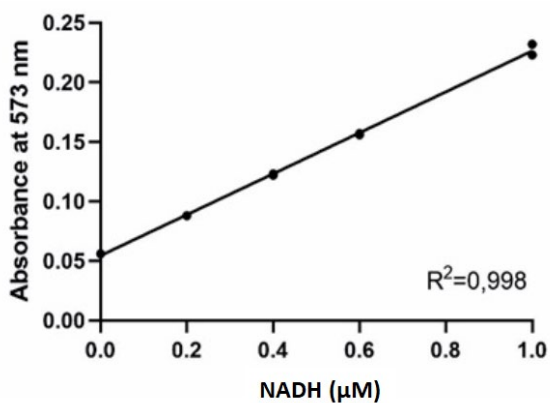

Standard	NADH (μM)	Absorbance (573 nm)
Assay time: 6 min		
ST1	0	0.056
ST2	0.2	0.088
ST3	0.4	0.122
ST4	0.6	0.157
ST5	1	0.223

C) CALCULATION OF RESULTS FOR NAD⁺

Concentration values in the stabilized sample extracts (UNK) and sample blanks (BL UNK1-4) are determined from the linear fit formula of the NAD⁺ standard curve.

Unknown	Concentration in stabilized extracts (μM)	Concentration in stabilized extracts corrected by average of sample blanks (BL UNK 1-4, μM)	Final NAD ⁺ concentration in the original sample (μM)*
UNK 1	2.944 3.151	3.008	30.08
UNK 2	2.841 3.129	2.945	29.45
UNK 3	2.686 2.730	2.668	26.68
UNK 4	1.895 1.999	1.907	19.07
UNK 5	2.346 2.420	2.343	23.43
UNK 6	3.432 3.499	3.425	34.25
BL UNK 1	0.040	-	
BL UNK 2	0.048		
BL UNK 3	0.026		
BL UNK 4	0.048		

*Corrected by dilution factor x10

D) CALCULATION OF RESULTS FOR NADH

Concentration values in the stabilized sample extracts (UNK) and sample blanks (BL UNK1-4) are determined from the linear fit formula of the NADH standard curve.

Unknown	Concentration in stabilized extracts (μM)	Concentration in stabilized extracts corrected by average of sample blanks (BL UNK 1-4, μM)	Final NADH concentration in the original sample (μM)*
UNK 1	0.239 0.239	0.086	0.86
UNK 2	0.284 0.290	0.133	1.33
UNK 3	0.228 0.234	0.077	0.77
UNK 4	0.234 0.239	0.083	0.83
UNK 5	0.200 0.195	0.044	0.44
UNK 6	0.228 0.245	0.083	0.83
BL UNK 1	0.156	-	
BL UNK 2	0.161		
BL UNK 3	0.150		
BL UNK 4	0.150		

*Corrected by dilution factor x10

PERFORMANCE AND LIMITATIONS

LIMITS OF DETECTION

The Limit of Blank (LoB) for Q-NAD Blood is presented in the table below (LoB $\pm$ standard deviation [SD]).

Limit of Blank (pmol/well)	
NAD+	1.84 $\pm$ 0.9
NADH	2.10 $\pm$ 0.5

The Limit of Detection (LoD) was calculated from NAD+ and NADH standard curves and is presented in the table below (LoD $\pm$ SD).

Limit of Detection (μ M in whole blood)	
NAD+	0.33 $\pm$ 0.2
NADH	0.19 $\pm$ 0.05

The Limit of Quantitation (LoQ) is presented in the table below (LoQ $\pm$ SD).

Limit of Quantitation (μ M in whole blood)	
NAD+	0.66 $\pm$ 0.3
NADH	0.40 $\pm$ 0.1

PRECISION AND REPRODUCIBILITY

Intra-assay variation in measurement determined the precision of the assay performance. The table below presents the intra-assay precision (CV=coefficient of variation).

Intra-assay precision (CV (%) $\pm$ SD)	
NAD+	1.48 $\pm$ 0.8
NADH	3.33 $\pm$ 1.5

The table below summarizes the results of the assay reproducibility.

Reproducibility

	NAD+			NADH		
Sample	Ctr1	Ctr2	Ctr3	Ctr1	Ctr2	Ctr3
N of measurements *	9	9	9	9	9	9
Mean (μ M)	27.41	29.41	22.00	0.55	0.71	0.64
Standard deviation	0.62	1.31	0.87	0.03	0.05	0.05
CV (%)	2.28	4.45	3.95	5.20	7.06	8.45

(N=number, * 3 aliquots of the same sample were analyzed in triplicates).

ACCURACY

The accuracy of the assay was calculated from samples with known amounts of pure NAD+ and NADH. The table below summarizes the results (assay accuracy +/- SD).

Accuracy (%)		
NAD+	N = 32	97.13 ± 7.6
NADH	N = 25	104.22 ± 16.5

ASSAY CUT-OFF

The low and high cut-off values represent the smallest and highest concentrations observed in 5-7% of Finnish individuals of a given population extract. The table below summarizes the cut-off values.

Cut-off value		
	Low	High
NAD+ (µM)	20	36
NADH (µM)	0.6	1.8


PERFORMANCE CHARACTERISTICS

The interference of other metabolites in the extract was not separately investigated, as their contribution is low and taken into account by performing the blank correction without added enzyme.

Warning: Potassium sorbate, borate, pyridine, and bismuth in a sample can cause enzyme inhibition, thus causing underestimation of the results.

METHOD VALIDATION

To validate the performance of NADMED, we measured NAD+ concentration in a set of control human blood samples that were also analyzed by mass spectrometry. Frozen blood samples of five healthy subjects (before and after 16 weeks of niacin supplementation) were analyzed in parallel by NADMED and mass spectrometry. Results from NADMED were concordant with those obtained by mass spectrometry.

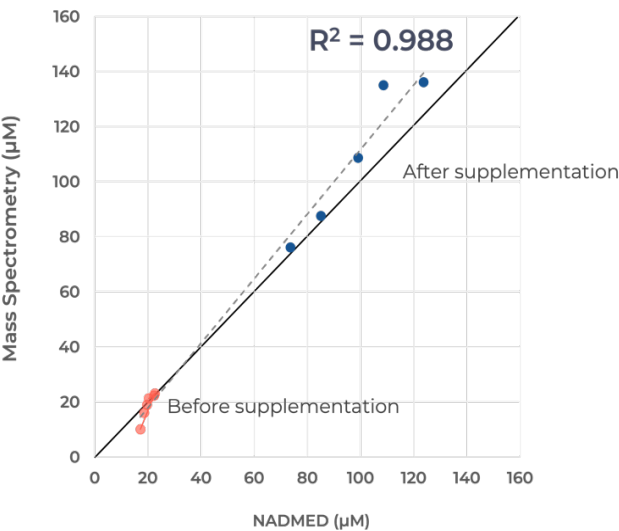

NOTES

[illegible]

PLATE LAYOUT

Use this plate layout to record your samples on the plate.

